



TR-09-91
Ottawa Police Department
**Radiation Measurements on the Police Traffic
Radar Speed Detectors**

L. Allan
MPB Technologies Inc.

TECHNICAL REPORT
November 1991

NOTE: Further information
about this report can be
obtained by calling the
CPRC information number
(613) 998-6342

Customer No.: 70670

MPBT No.: 1126

**Test Report for
Radiation Measurements
on the
Police Traffic Radar
Speed Detectors**

L. Allan

Prepared for:

OTTAWA POLICE
474 Elgin Street
Ottawa, Ontario
K2P 2J6

Prepared by:

MPB Technologies Inc.
Building M-50, NRC
Montreal Road
Ottawa, Ontario
K1A 0R6

November 26, 1991
03-R-126 (MS)



Dave G. Scribailo
Manager
Electromagnetic Services
Electromagnetics Division

TABLE OF CONTENTS

1.0 Summary of Radar Measurements

2.0 Radar Measurements

3.0 Calibration Certificates

APPENDICES

Appendix A: Power Density Table

Appendix B: Radiation Patterns

Appendix C: Test Equipment Report

Appendix D: Bibliography

1.0 SUMMARY OF RADAR MEASUREMENTS

SUMMARY


The Safety Code - 6 of National Health and Welfare states that the "General Public (those individuals that are not microwave radiation workers) shall not be exposed to power density levels greater than one (1) mW/cm² averaged over a one-minute period in the range of frequencies between 10 MHz and 300 GHz.

Units #30 (13299) and #28 (13301) operate on CW (continuous wave) and are well below the one (1) mW/cm².

The remaining units operate on a 40% duty cycle. The radiated power would be 40% of the measured value with a possible error of +20% -17%.

All units passed, with #12 (6659) being borderline at two (2) inches.

$$\text{ie: } 2.14 \text{ mW/cm}^2 \cdot 40\% \cdot 120\% = 1.0 \text{ mW}$$



2.0 RADAR MEASUREMENTS

OTTAWA POLICE RADAR SPEED DETECTORS

The radiation levels at 10.524 GHz were checked at two (2) and six (6) inches from the horn cover.

A small linear horn (2.5 cm x 2.25 cm mouth) was used to receive the radiated energy. The Horn was first calibrated, using an HP8510 Network Analyzer. With the three-antenna system, the gain of the Horn measured 9 dB. The expected power from the Horn in a 1-mW/cm² field was determined by the formula:

$$Pr = \frac{F \cdot G \cdot \lambda^2}{4 \pi}$$

Pr = Power Received

F = Field mW/cm² at the Horn focus

G = Gain of Horn

λ = Wavelength at 10.524 GHz

$$\text{ie: } Pr = \frac{1 \text{ mW/cm}^2 \times 9 \times (2.849\text{cm})^2}{4 \pi} = 5.8 \text{ mW}$$

A calibrated source of 10.524 GHz was set to 5.8 mW and fed into a receiver. The Receiver signal was noted and compared to the signals from the Horn when the Horn was placed two (2) and six (6) inches from the radars. Since the radars transmit circular polarized signals, the vertical and horizontal signal from the Horn were added. The results are shown in Table 1.

Note 1:

For measurements, all radars were set to CW operation. If the radars are modulated OFF and ON, the average radiation power will be reduced in the same ratio as of the ON and OFF time.

Note 2:

The overall accuracy of the measurement was + 0.8 dB or +20% -17%.

Note 3:

Some radiation patterns have been included for general information.

3.0 CALIBRATION CERTIFICATES



MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-C1
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni-Coupe
Model No.: 1MDR-1 Serial No.: 13299
Calibration Date: November 26, 1991 Calibration Due: November 25, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 8566B.	92-061321.
HP Network Analyzer 8510A	92-060521.
Weinschel 10dB Attenuator 861. (P5027)	92-080121.
Weinschel 10dB Attenuator 861. (R1696)	92-080122.
HP Power Meter 432B.	N/A
HP Thermistor Mount. 84782.	N/A.
HP Directional Coupler 11691D.	N/A.
Scientific Atlanta Harmonic Mixer 14-5.	N/A.
SA Harmonic Mixer 14-5 (104010C)	N/A.
HP Adapter X201A.	N/A.
Pro Tuner 303. (238 + 456)	N/A.
Harrison Lab Power Supply 505A.	N/A.
SA Antenna Positioner RMA-3-1.	N/A.
NRC Standard Gain Horn.	N/A.
HP Computer 23c.	N/A.

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date:

MPB Technologies Inc.:

November 26, 1991



HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "E M Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/- 2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. SW1000

Manager, Electromagnetic Services





MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-A2
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni-Quip
Model No.: T3 Serial No.: 5806
Calibration Date: November 20, 1991 Calibration Due: November 20, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 2566B	92-061321.
HP Network Analyzer 2510A	92-060521.
Weinschel 10dB Attenuator Pad (P5027)	92-080121
Weinschel 10dB Attenuator Pad. (R1696)	92-080122.
HP Power Meter 432B.	N/A
HP Thermistor Mount 8478A.	N/A.
HP Directional Coupler 11691D	N/A
SA Harmonic Mixer 14-5(483)	N/A
SA Harmonic Mixer 14-5(104810C)	N/A
HP Adapter X281A.	N/A
ProTuner 303(238 & 456).	N/A
HarrisonLab Power Supply 505A	N/A
SA Antenna Positioner PMA-3-1.	N/A
NRC Standard Gain Horn.	N/A
HP Computer 236.	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991
MPB Technologies Inc.: November 26, 1991



MPB TECHNOLOGIES INC.

HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "E M Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility, Radiated Emission Measurement in EMI, Calibration of Antennas" 1988
- SAE-ARP 958: "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/-2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. SW1000

Manager, Electromagnetic Services



CANADA
AWARDS FOR
BUSINESS
EXCELLENCE
Montreal
Quebec
Canada





MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-03
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TABAR Muni-Quiip
Model No.: T3 Serial No.: 55060
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 2566B	92-061321
HP Network Analyzer 8510A	92-C60521
Weinschel 10dB Attenuator Pad (P5027)	92-080121
Weinschel 10dB Attenuator Pad (R1696)	92-080122
HP Power Meter 432B	N/A
HP Thermistor Mount 84781	N/A
HP Directional Coupler 11691D	N/A
SA Harmonic Mixer 14-5(483)	N/A
SA Harmonic Mixer 14-5(104810C)	N/A
HP Adapter X281A	N/A
ProTuner 303(232+456)	N/A
Harrison Lab Power Supply 505A	N/A
SA Antenna Positioner RINH-3-1	N/A
NRC Standard Gain Horn	N/A
HP Computer 236	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991

MPB Technologies Inc.: November 26, 1991



HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "E M Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/- 2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. SW1000

Manager, Electromagnetic Services



CAN/AM
AWARDS FOR
BUSINESS
EXCELLENCE
Montreal, Quebec, Canada
October 1992





MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-OK
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Mun.-Quip.
Model No.: T3 Serial No.: 5802
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 2566B	92-061321
HP Network Analyzer 8510A	92-060521
Weinschel 10dB Attenuator Pad (P5027)	92-080121
Weinschel 10dB Attenuator Pad (R1696)	92-080122
HP Power Meter 432B	N/A
HP Thermistor Mount 8478A	N/A
HP Directional Coupler 11691D	N/A
SA Harmonic Mixer 14-5(483)	N/A
SA Harmonic Mixer 14-5(104810C)	N/A
HP Adapter X281A	N/A
Pro Tuner 303(238 + 456)	N/A
Harrison Lab Power Supply 5051A	N/A
SA Antenna Positioner PMA-3-1	N/A
NRC Standard Gain Horn	N/A
HP Computer 236	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991

MPB Technologies Inc.: November 26, 1991



HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.
Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "E M Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/-2 dB

- CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).
- ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

- EQUIPMENT USED: HP Network Analyzer Model No. 8510
Advantest Spectrum Analyzer Model No. R3261A
Rohde & Schwarz Signal Generator Model No. SWP
AR Amplifier Model No. SW1000

Manager, Electromagnetic Services



CANADA
AWARDS FOR
BUSINESS
EXCELLENCE
Entrepreneurial
Excellence
Program





MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-05
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni-Quip
Model No.: T3. Serial No.: 6659
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 8566B.	92-061321.
HP Network Analyzer 8510A.	92-060521.
Weinschel 10dB Attenuator Pad (P5027).	92-080121.
Weinschel 10dB Attenuator Pad (R1696).	92-080122.
HP Power Meter 432B.	N/A
HP Thermistor Mount 8478A.	N/A
HP Directional Coupler 11691D.	N/A
SA Harmonic Mixer 14-5(423)	N/A
SA Harmonic Mixer 14-5(104810C)	N/A
HP Adapter X281A	N/A
ProTuner 303(238+456)	N/A
Harrisonlab Power Supply 505A	N/A
SA Antenna Positioner PMA-3-1.	N/A
NRC Standard Gain Horn.	N/A
HP Computer 236.	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991
MPB Technologies Inc.: November 26, 1991



HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "EM Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility, Radiated Emission Measurement in EMI, Calibration of Antennas" 1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"


CALIBRATION ACCURACY: +/-2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. SW1000

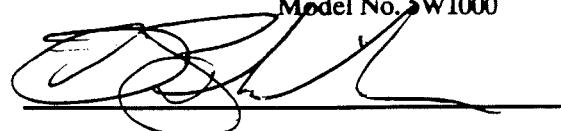

Manager, Electromagnetic Services



MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-06
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni-Quip
Model No.: MDR-1 Serial No.: 13301
Calibration Date: November 20, 1991 Calibration Due: November 20, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 8566B	92-061321
HP Network Analyzer 8510A	92-060521
Weinschel 10dB Attenuator Pad (P5027)	92-080121
Weinschel 10dB Attenuator Pad (R1696)	92-080122
HP Power Meter 432B	N/A
HP Thermistor Mount .8478A	N/A
HP Directional Coupler 11691D	N/A
SA Harmonic Mixer 14-5 (483)	N/A
SA Harmonic Mixer 14-5 (104810C)	N/A
HP Adapter X281A	N/A
ProTuner 303(238 + 456)	N/A
Harrison Lab Power Supply .505A	N/A
SA Antenna Positioner PMA-3-1	N/A
NRC Standard Gain Horn	N/A
HP Computer 236	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991

MPB Technologies Inc.: P. Brown - 1126



MPB TECHNOLOGIES INC.

HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "E M Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz,J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"


CALIBRATION ACCURACY: +/- 2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. 5W1000

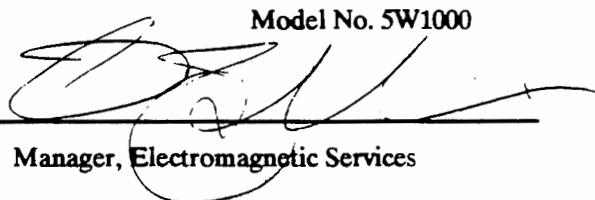

Manager, Electromagnetic Services



MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-07
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni - Quip
Model No.: 13 Serial No.: 5810
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 2566B.	92-061321.
HP Network Analyzer 2510A	92-060521.
Weinschel 10dB Attenuator Pad (P5027)	92-080121.
Weinschel 10dB Attenuator Pad (R16916).	92-080122.
HP Power Meter 4328.	N/A
HP Thermistor Micro 8478A.	N/A
HP Directional Coupler 11691D	N/A
SA Harmonic Mixer 14-5(483)	N/A
SA Harmonic Mixer 14-5(104810C.)	N/A
HP Hdiptcr X2812	N/A
Pro Tuner 303 (238+456)	N/A
Harrison Lab Power Supply 505A	N/A
SA Antenna Positioner (PMA-3-1)	N/A
NRC Standard Gain Horn	N/A
HP Computer 236	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991

MPB Technologies Inc.: John ... 11-12



HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "E M Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/- 2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. SW1000

Manager, Electromagnetic Services





MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26, 1991 Calibration No.: 1126-08
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni - Quip
Model No.: 13 Serial No.: 6656
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 8566B.	92-061321.
HP Network Analyzer 2510A.	92-060521.
Weinschel 10dB Attenuator Pad (P5027).	92-080121.
Weinschel 10dB Attenuator Pad (R1696).	92-080122.
HP Power Meter 432B.	N/A
HP Thermistor Mount 8478A.	N/A
HP Directional Coupler 11691D.	N/A
SA Harmonic Mixer 14-5(483)	N/A.
SA Harmonic Mixer 14-5(104810C).	N/A.
HP Adapter X281A.	N/A
Pro Tuner 303(238+456)	N/A
Harrison Lab Power Supply 505A	N/A
SA Antenna Positioner PMA-3-1.	N/A
NRC Standard Gain Horn.	N/A.
HP Computer 236.	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991.

MPB Technologies Inc.: RECEIVED SERIALIZED



MPB TECHNOLOGIES INC

HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.
Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "EM Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/- 2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the
National Institute of Standards and Technology (NIST)
and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. 5W1000

Manager, Electromagnetic Services





MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

CALIBRATION CERTIFICATE

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November Calibration No.: 1126-09
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni-Quiq
Model No.: T3 Serial No.: 6903
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 8566B.	92-061321
HP Network Analyzer 8510A	92-060521
Weinschel 10dB Attenuator Pad (P5027)	92-080121
Weinschel 10dB Attenuator Pad (R1696)	92-080122
HP Power Meter 432B.	N/A.
HP Thermistor Mount 8478A.	N/A.
HP Directional Coupler 11691D.	N/A.
SA Harmonic Mixer 14-5(483)	N/A.
SA Harmonic Mixer 14-5(104810C)	N/A.
HP Adapter X261A	N/A.
ProTuner 303(238+456)	N/A.
Harrison Lab Power Supply 505A	N/A.
SA Antenna Positioner PMA-3-1	N/A.
NRC Standard Gain Horn.	N/A.
HP Computer 236.	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991

MPB Technologies Inc.:



HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.
Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "EM Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility, Radiated Emission Measurement in EMI, Calibration of Antennas" 1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/- 2 dB

CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the National Institute of Standards and Technology (NIST) and to the National Research Council of Canada (NRCC).

ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

EQUIPMENT USED:	HP Network Analyzer	Model No. 8510
	Advantest Spectrum Analyzer	Model No. R3261A
	Rohde & Schwarz Signal Generator	Model No. SWP
	AR Amplifier	Model No. SW1000

Manager, Electromagnetic Services





CALIBRATION CERTIFICATE

MPB Technologies Inc.
Electromagnetics Division
P.O. Box 9722 Station T
Ottawa, Ontario K1G 4X9

Telephone: (613) 744-3273
Fax: (613) 952-7998

Date: November 26 1991 Calibration No.: 1126-10
Company: Ottawa Police P.O. No.: 70670
Equipment Type: TRIBAR Muni-Quiq
Model No.: T3 Serial No.: 7324
Calibration Date: November 21, 1991 Calibration Due: November 21, 1992

Standard Used	Traceability No.
HP Spectrum Analyzer 8566B	92-061321
HP Network Analyzer 8510A	92-060521
Weinschel 10dB Attenuator Pad (P5027)	92-080121
Weinschel 10dB Attenuator Pad (R16916)	92-080122
HP Power Meter 432B	N/A
HP Thermistor Mount 8478A	N/A
HP Directional Coupler 11691D	N/A
SA Harmonic Mixer 14-5(483)	N/A
SA Harmonic Mixer 14-5(104810C)	N/A
HP Adapter X261A	N/A
Pro Tuner 303(238+456)	N/A
Harrison Lab Power Supply 505A	N/A
SA Antenna Positioner PMA-3-1	N/A
NRC Standard Gain Horn	N/A
HP Computer 236	N/A

This is to certify that the instrument listed above was calibrated to MPB Technologies Inc. standards which are traceable to the National Institute of Standards and Technology to the extent allowed by the Institutes calibration facilities, or to the National Research Council, to the extent allowed by the Councils calibration facilities.

Date: November 26, 1991

MPB Technologies Inc.: 1000000000000000



MPB TECHNOLOGIES INC.

HEAD OFFICE
1725 North Service Road
Trans-Canada Highway
Dorval, Quebec H9P 1J1
Telephone: (514) 683-1490
Fax: (514) 683-1727

LABORATORIES
151 Hymus Boulevard
Pointe Claire, Quebec
H9R 1E9
Telephone: (514) 694-8751
Fax: (514) 695-7492

ELECTROMAGNETICS
MEASUREMENT FACILITY
NRC, Montreal Road Building M-50
Ottawa, Ontario K1A 0R6
Telephone: (613) 744-3273
Fax: (613) 952-7998

ANTENNA CALIBRATION

MPB Technologies uses one or more of the following standard procedures to calibrate antennae.

Monopole and Loop Antennae:

- NBS: Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a TEM Cell"
Ref: Kanda, M.; Orr, R. David
- NRCC: "Measurement of Antenna Factors with a TEM Cell"
Ref: Kashyap, S.C.
- ECSM: "The Equivalent Capacitance Substitution Method"
Ref: Jordan, E.C., "EM Waves & Radiating System", p.483
Ref: Navship 94810, "The Radio Freq. Interference Meter",
Univ. of Penn., 1962, Para. 12.4.1
- IEEE 302-1969: "The Institute of Electrical and Electronic Engineers",
Sect. 2.2.2.3

Dipole, Dipole Array, Horn Antenna:

- NBS: Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas (25 to 1000 MHz)"
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5: "American National Standards for Electromagnetic Compatibility,
Radiated Emission Measurement in EMI, Calibration of Antennas"
1988
- SAE-ARP 958 "Broadband Electromagnetic Interference Measurement Antennas; Standard Calibration Requirements and Methods"

CALIBRATION ACCURACY: +/- 2 dB


- CALIBRATION TRACEABILITY: All Measurement Instrumentation traceable to the
National Institute of Standards and Technology (NIST)
and to the National Research Council of Canada (NRCC).
- ENVIRONMENT: Temperature: -10 to 35 degrees Centigrade
Humidity: 10 to 90% (Non-Condensing)

RE-CERTIFICATION DATE: 1 year from Calibration Date

- EQUIPMENT USED: HP Network Analyzer Model No. 8510
Advantest Spectrum Analyzer Model No. R3261A
Rohde & Schwarz Signal Generator Model No. SWP
AR Amplifier Model No. SW1000

Manager, Electromagnetic Services

APPENDIX A




**POWER DENSITY
AT 2 TO 6 INCHES FROM ANTENNA FACE**

Table 1

UNIT #	SPACING (INCHES)	POWER (mW/cm ²)
T ₃ 55060 #27	2	0.76
	6	0.66
T ₃ 5810 # 08	2	0.84
	6	0.76
T ₃ 6656 # 09	2	0.82
	6	0.66
T ₃ 6905 # 19	2	0.93
	6	0.78
T ₃ 5807 # 05	2	1.45
	6	1.35
Muni-Quip 6659 # 12	2	2.14
	6	1.23
T ₃ 5806 # 04	2	1.68
	6	1.51
T ₃ 7324 # 23	2	1.29
	6	1.15
MDR-1 13299 # 30	2	0.75
	6	0.69
MDR-1 13301 # 28	2	0.69
	6	0.58


APPENDIX B






Technologies Inc.

RADIATION PATTERN MEASUREMENT
CALIBRATION 5 dB STEPS

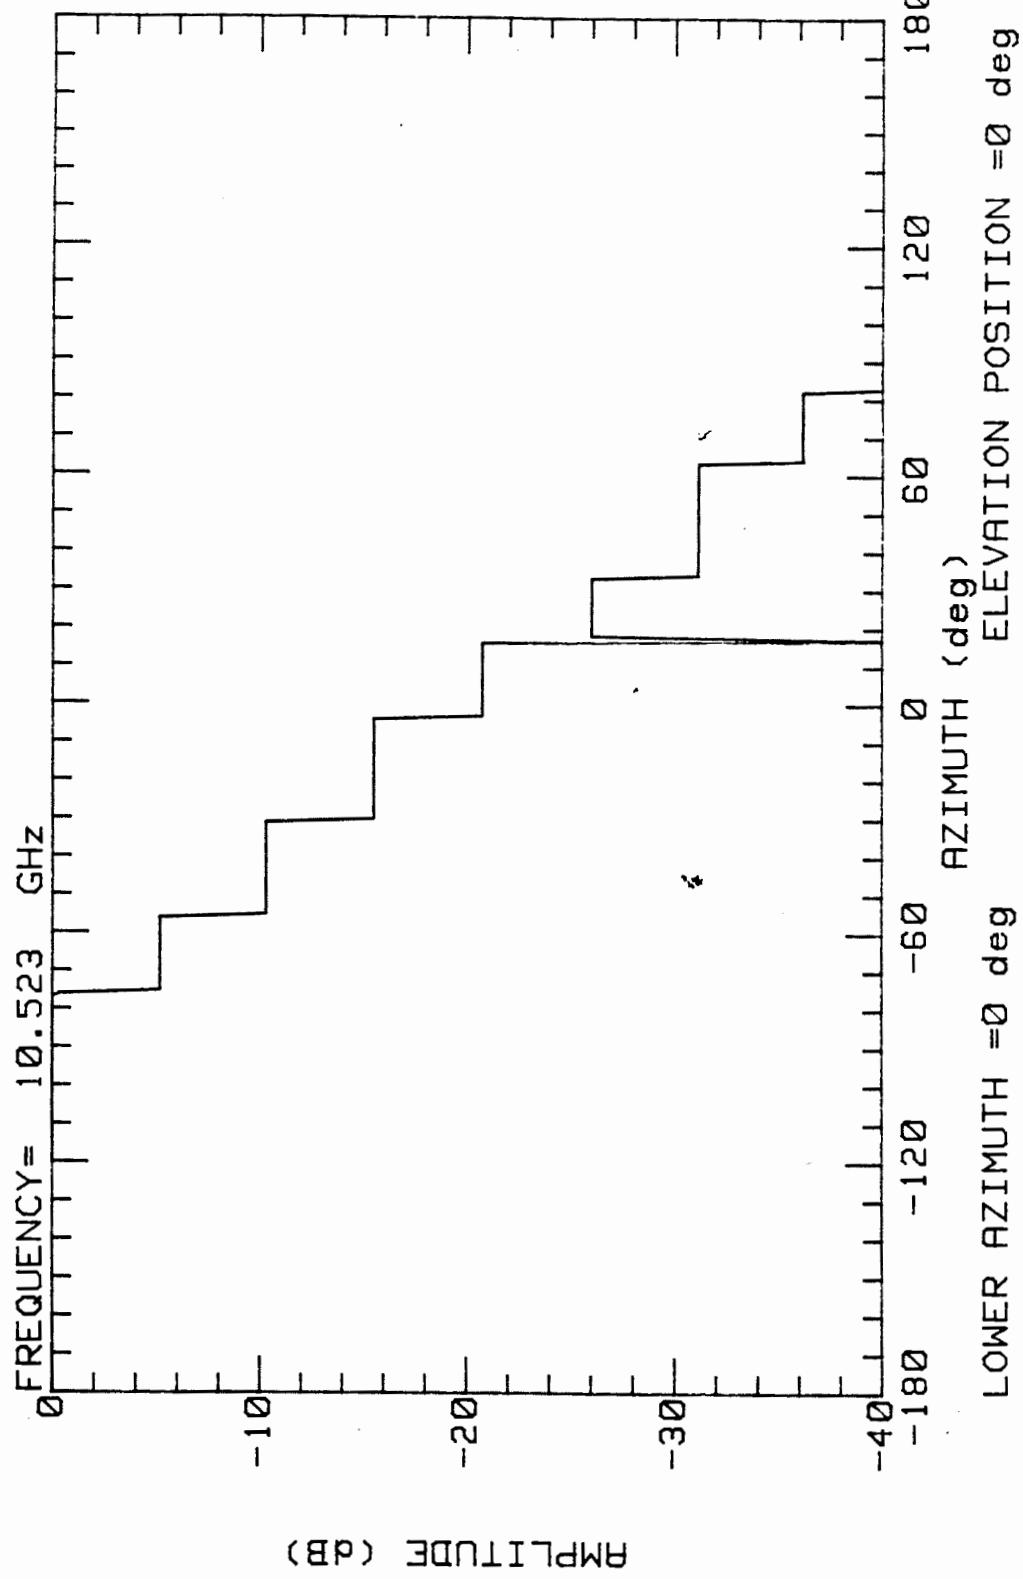

MPB
TECHNOLOGIES INC.

RADIATION PATTERN MEASUREMENT
TRIBAR INDUSTRIES MUNI QUIP MDR-1 #13299 Rx V
2 INCH SPACING
FREQUENCY = 10.523 GHz

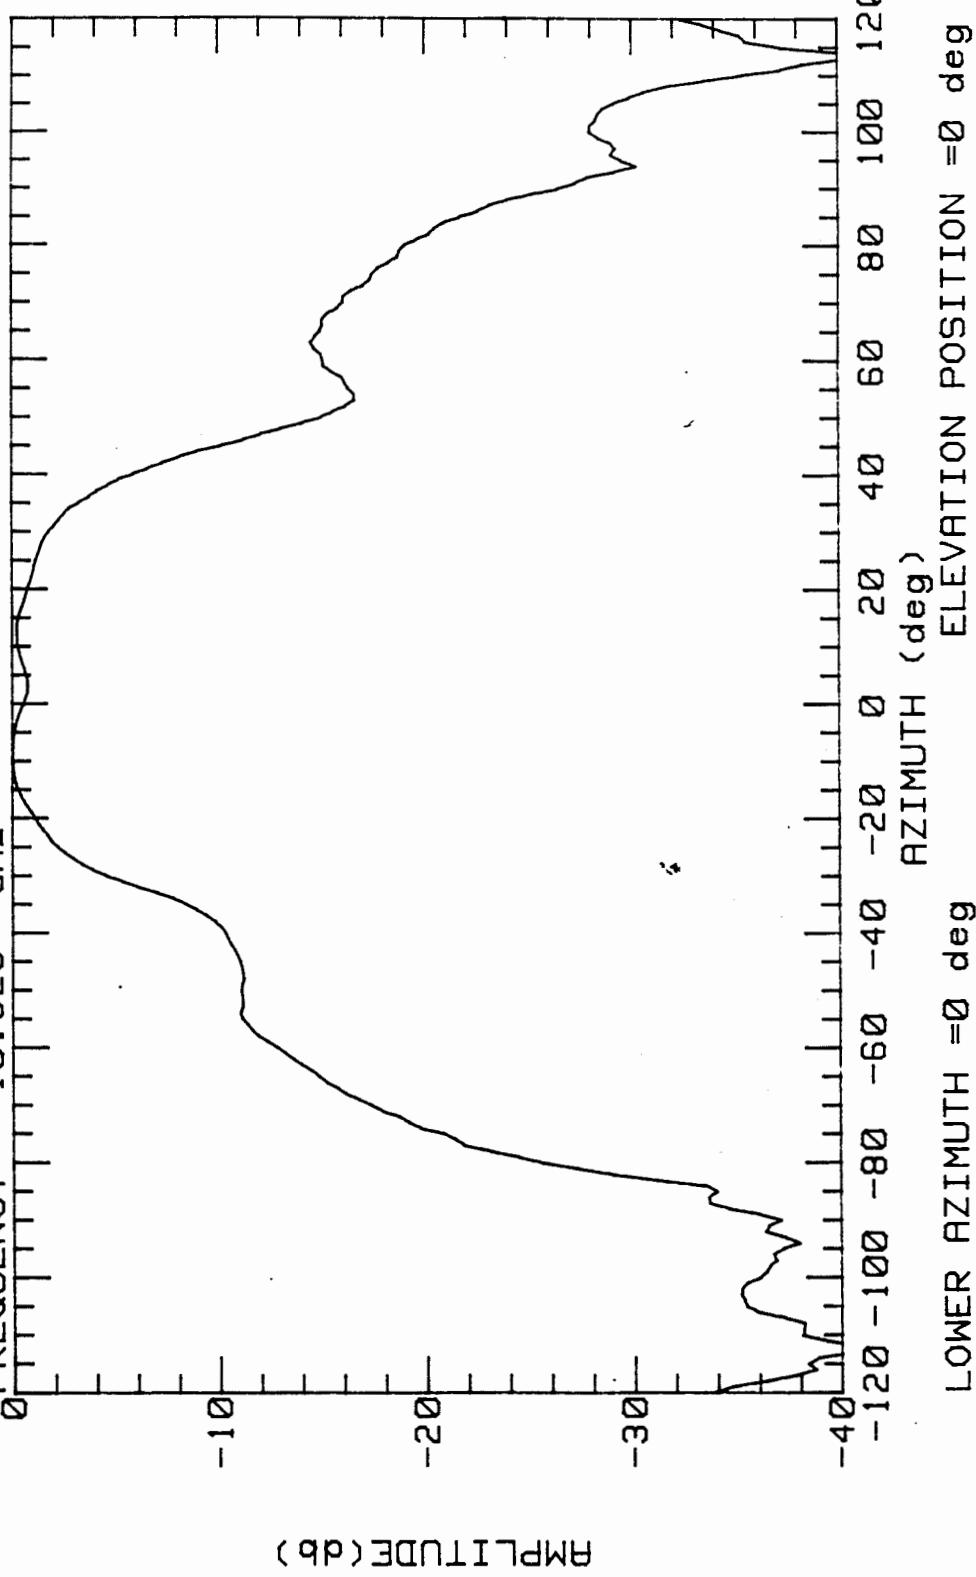


LOWER AZIMUTH = 0 deg
ELEVATION POSITION = 0 deg

NPB
TECHNOLOGIES INC.

RADIATION PATTERN MEASUREMENT

TRIBAR INDUSTRIES MUNI QUIP MDR-1 #13299 Rx V
6 INCH SPACING

FREQUENCY = 10.523 GHz

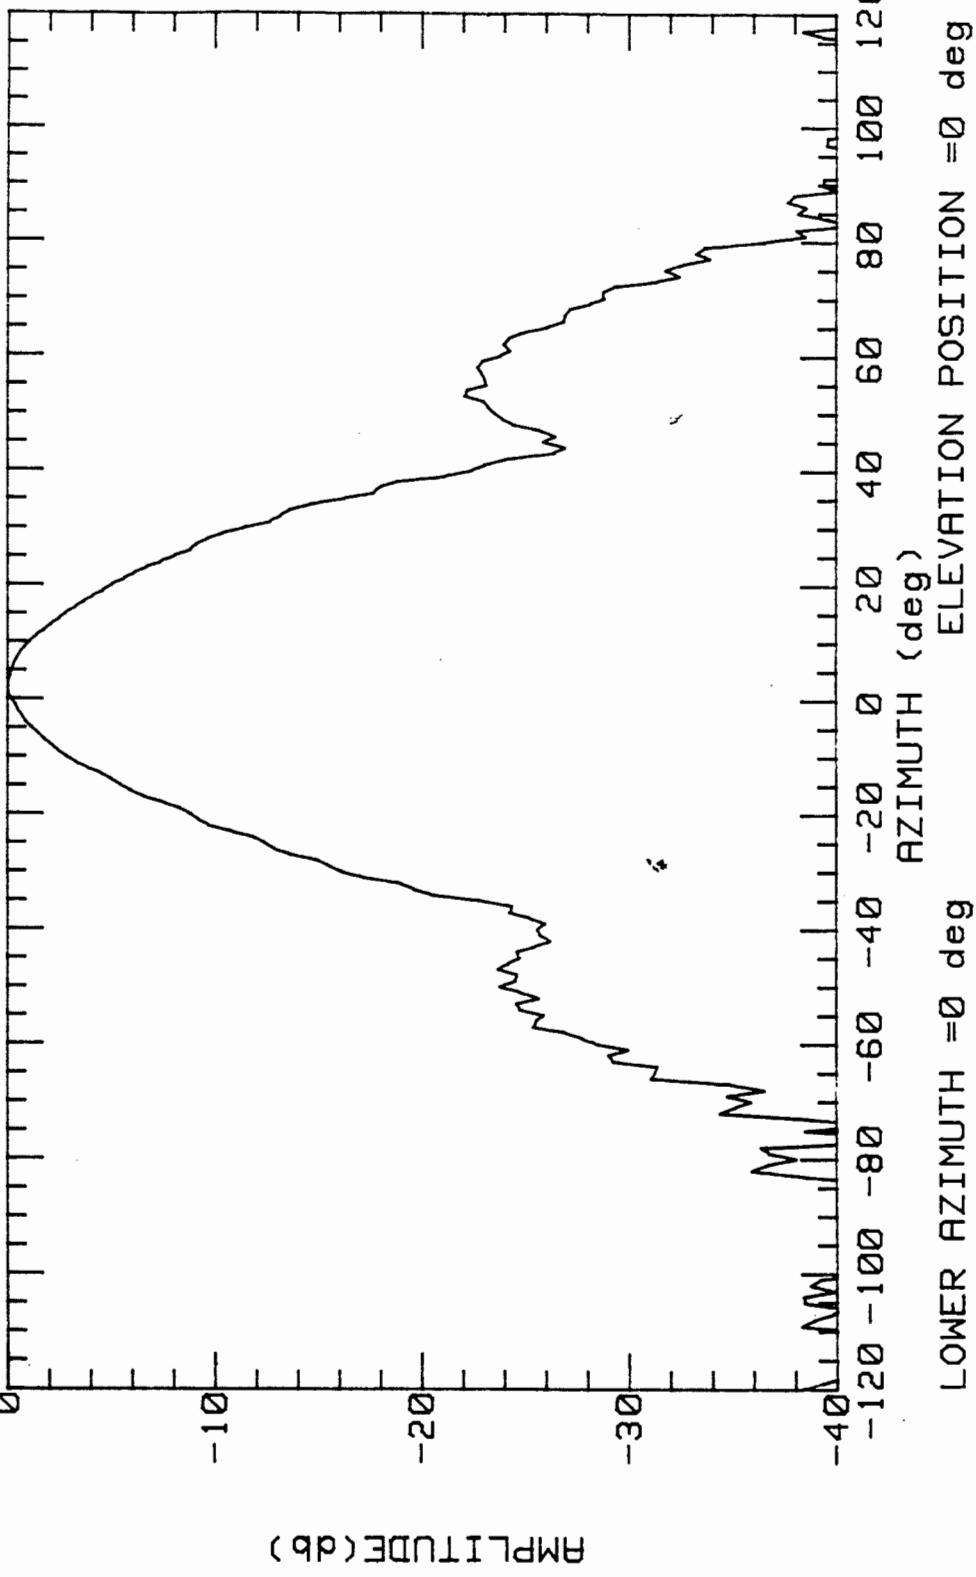


NPB TECHNOLOGIES INC. Exp.4SCAN 1 BY:

ON 20 Nov 1991 13:47:57

TRIBAR
TECHNOLOGIES INC.

RADIATION PATTERN MEASUREMENT
TRIBAR INDUSTRIES MUNI QUIP T3 #5806 -4
2 INCH SPACING
FREQUENCY = 10.523 GHz

AMPLITUDE (dB)

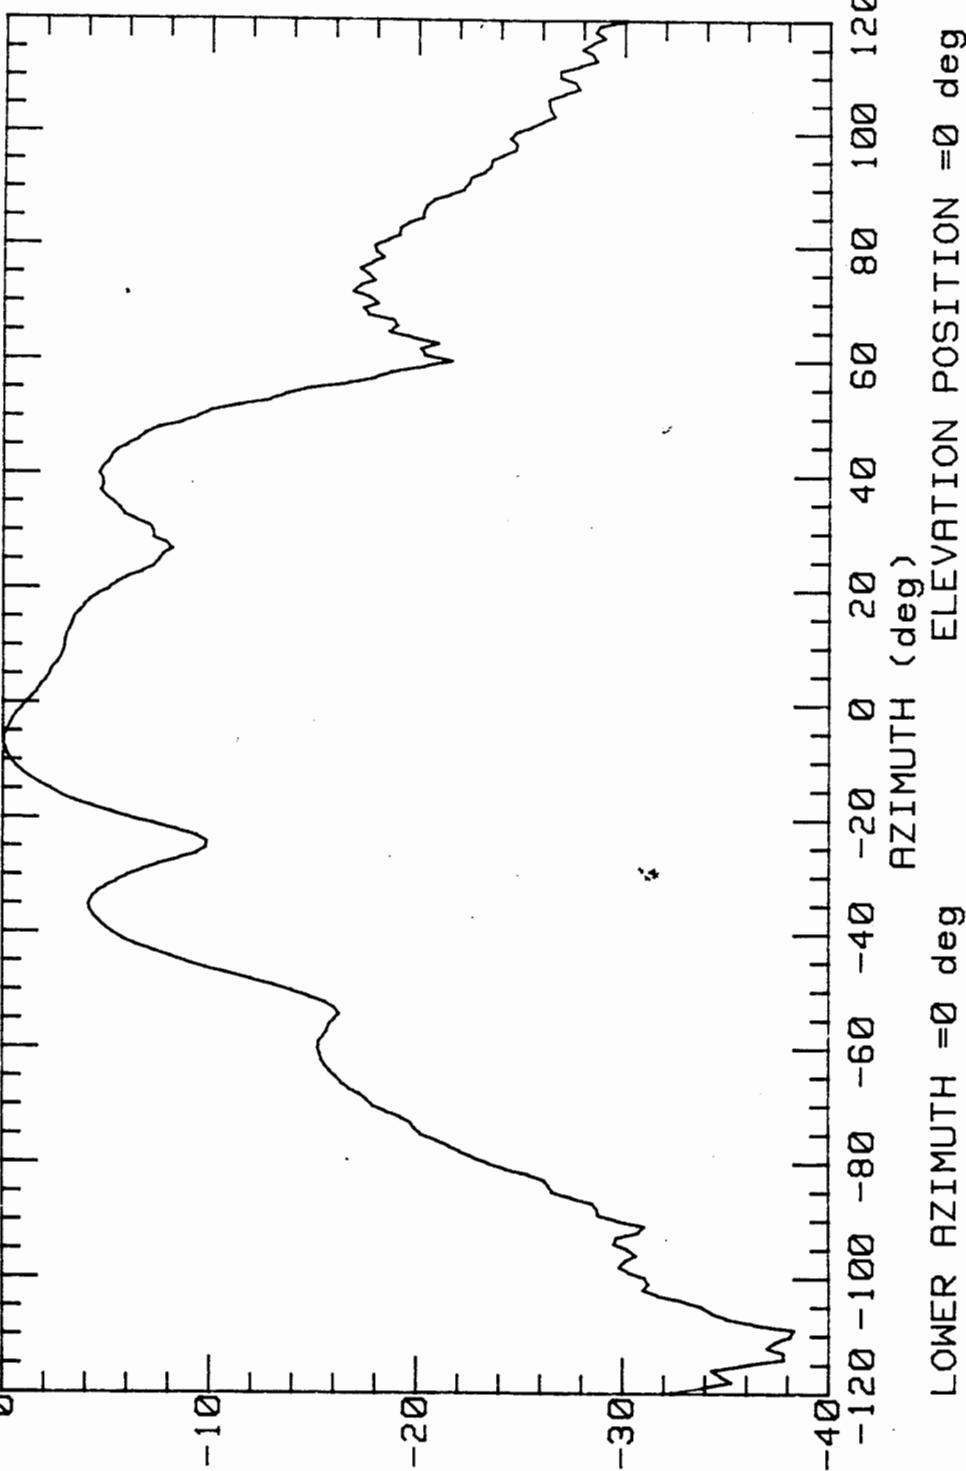


LOWER AZIMUTH = 0 deg
ELEVATION POSITION = 0 deg

TRIBAR
Technologies Inc.

RADIATION PATTERN MEASUREMENT

TRIBAR INDUSTRIES MUNI QUIP T3 #5806
6 INCH SPACING Rx H


FREQUENCY = 10.523 GHz

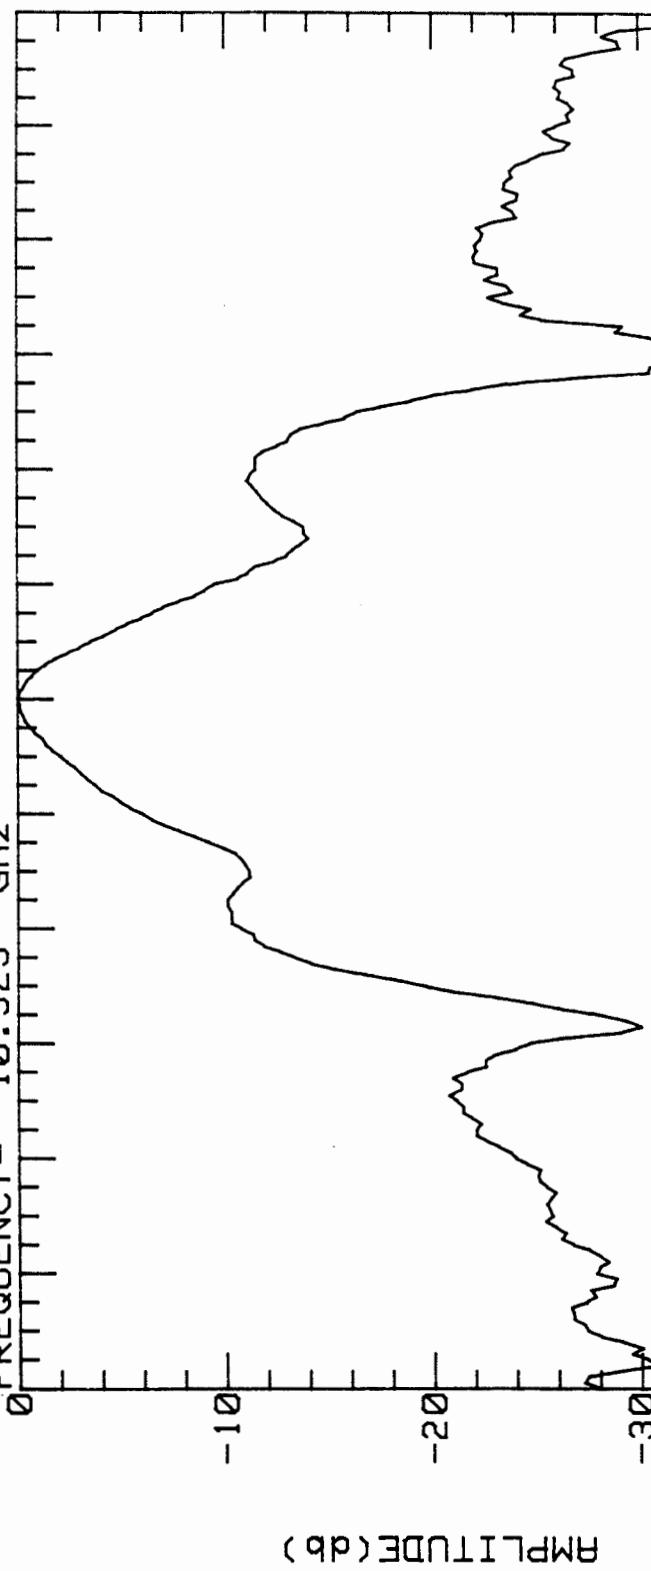

AZIMUTH (deg)
ELEVATION POSITION = 0 deg
LOWER AZIMUTH = 0 deg

MPB
TECHNOLOGIES Inc.

RADIATION PATTERN MEASUREMENT
TRIBAR INDUSTRIES MUNI QUIP T3 #5806 -4
2 INCH SPACING
FREQUENCY = 10.523 GHz

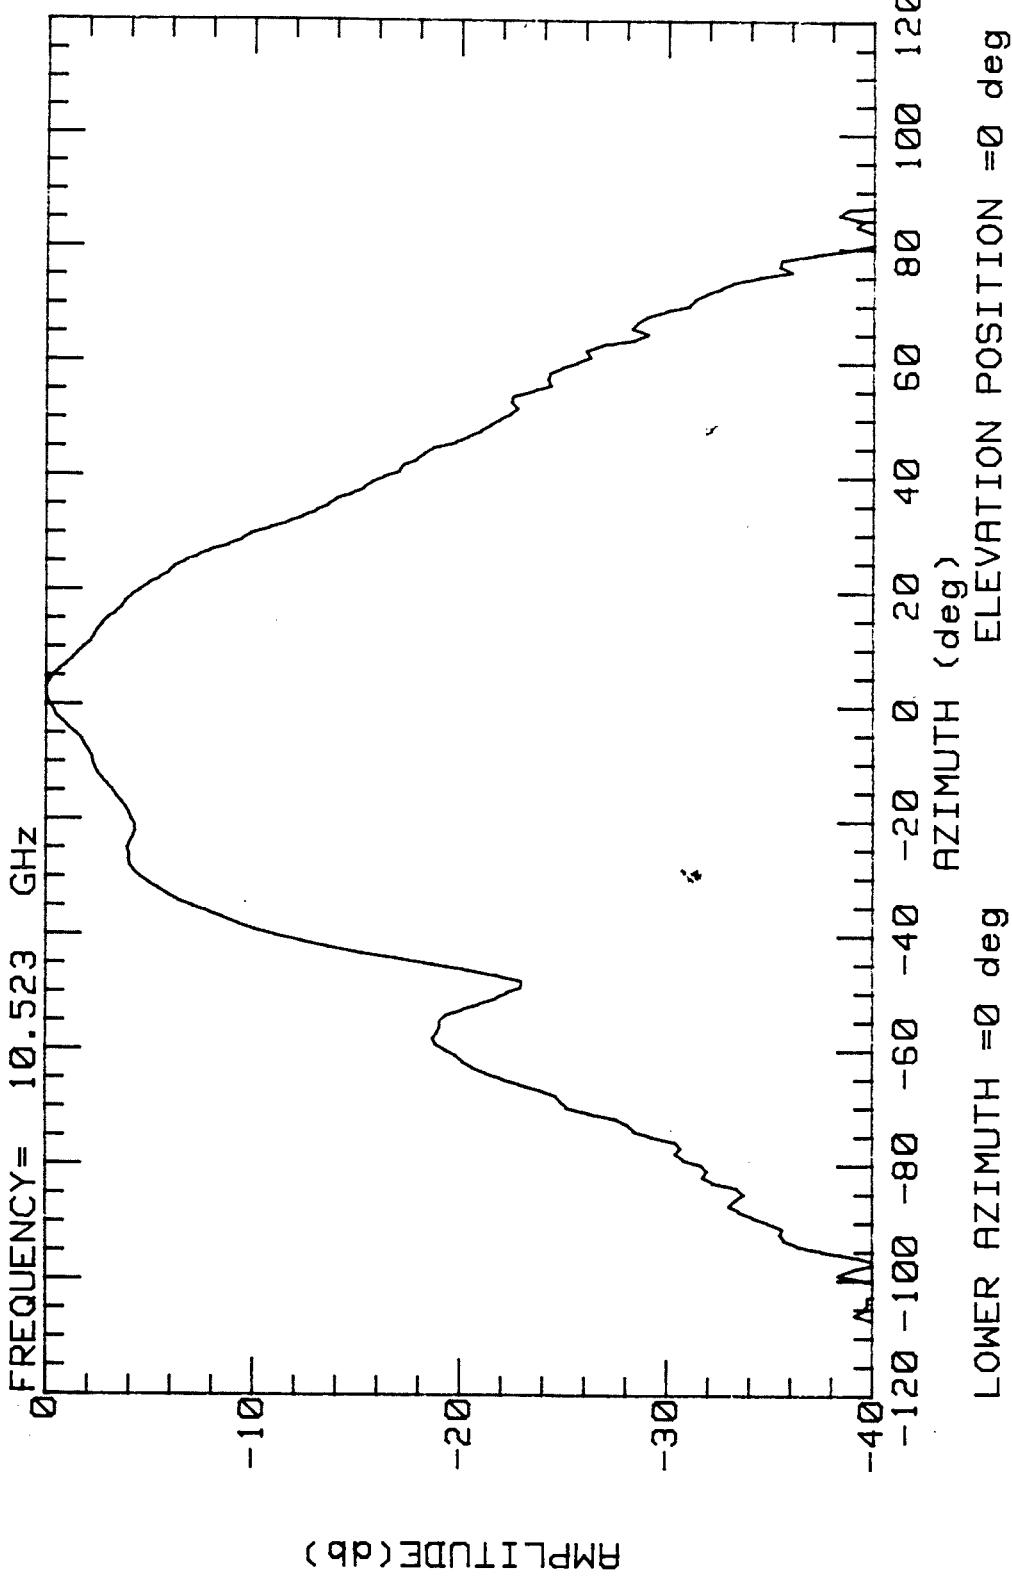




TRIBAR INDUSTRIES MUNI QUIP T3
6 INCH SPACING
FREQUENCY = 10.523 GHz


RADIATION PATTERN MEASUREMENT

#5806
Rx V

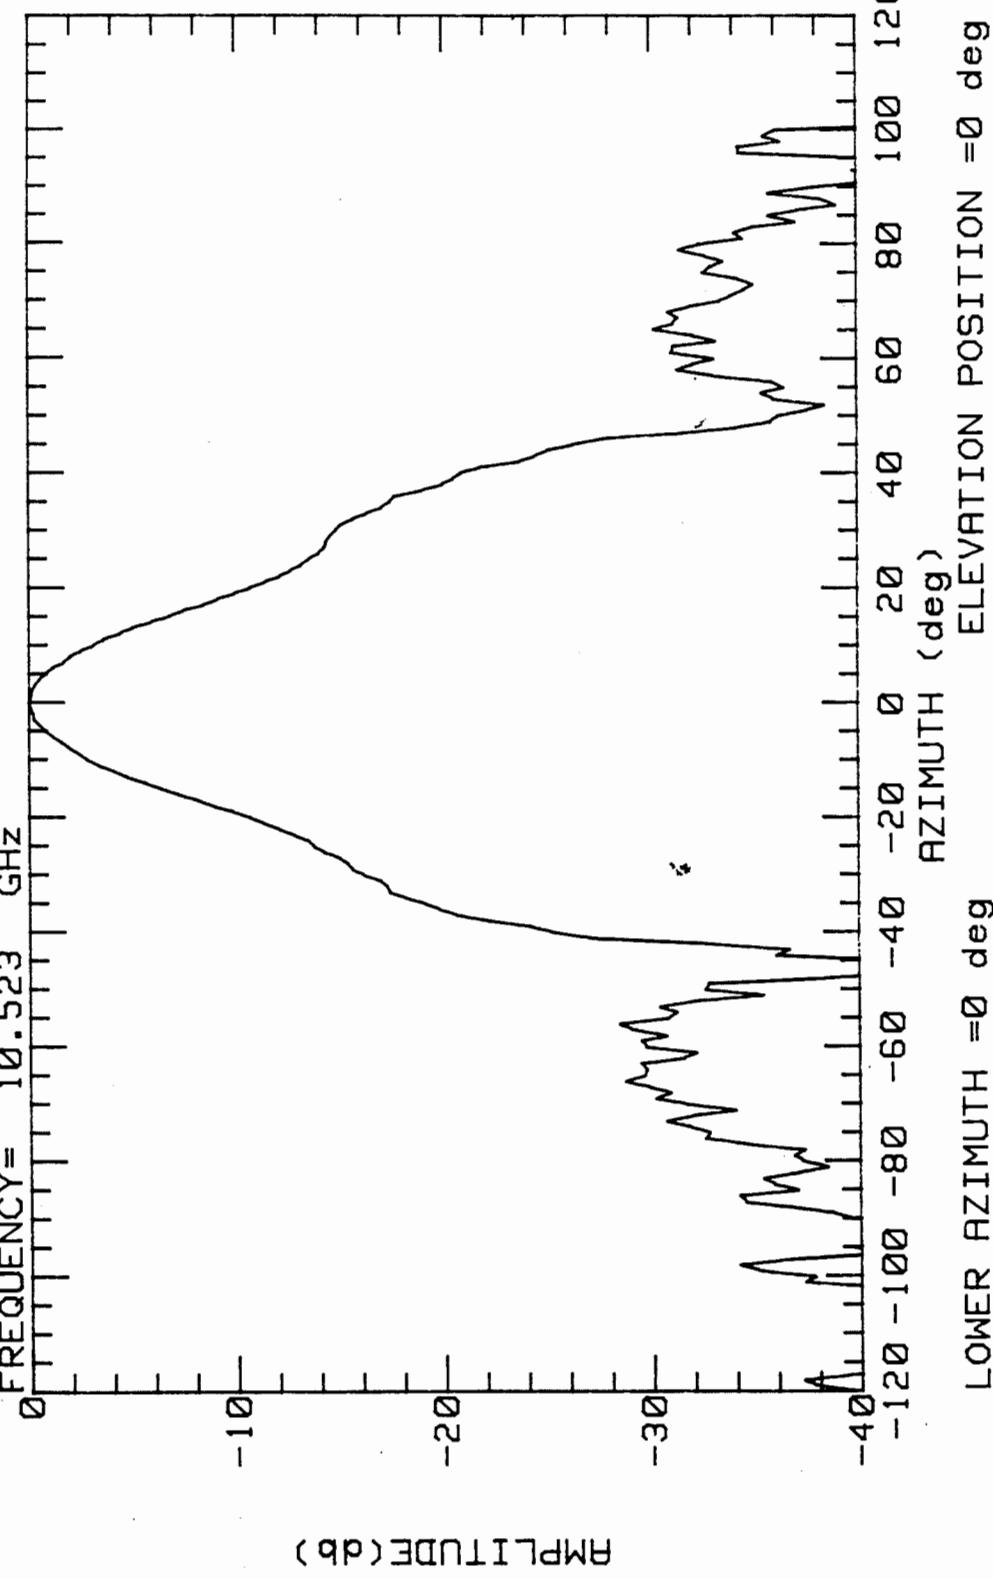

MPB
Technologies Inc.

RADIATION PATTERN MEASUREMENT
TRIBAR INDUSTRIES MUNI QUIP T3 #55060 -27
2 INCH SPACING Rx H

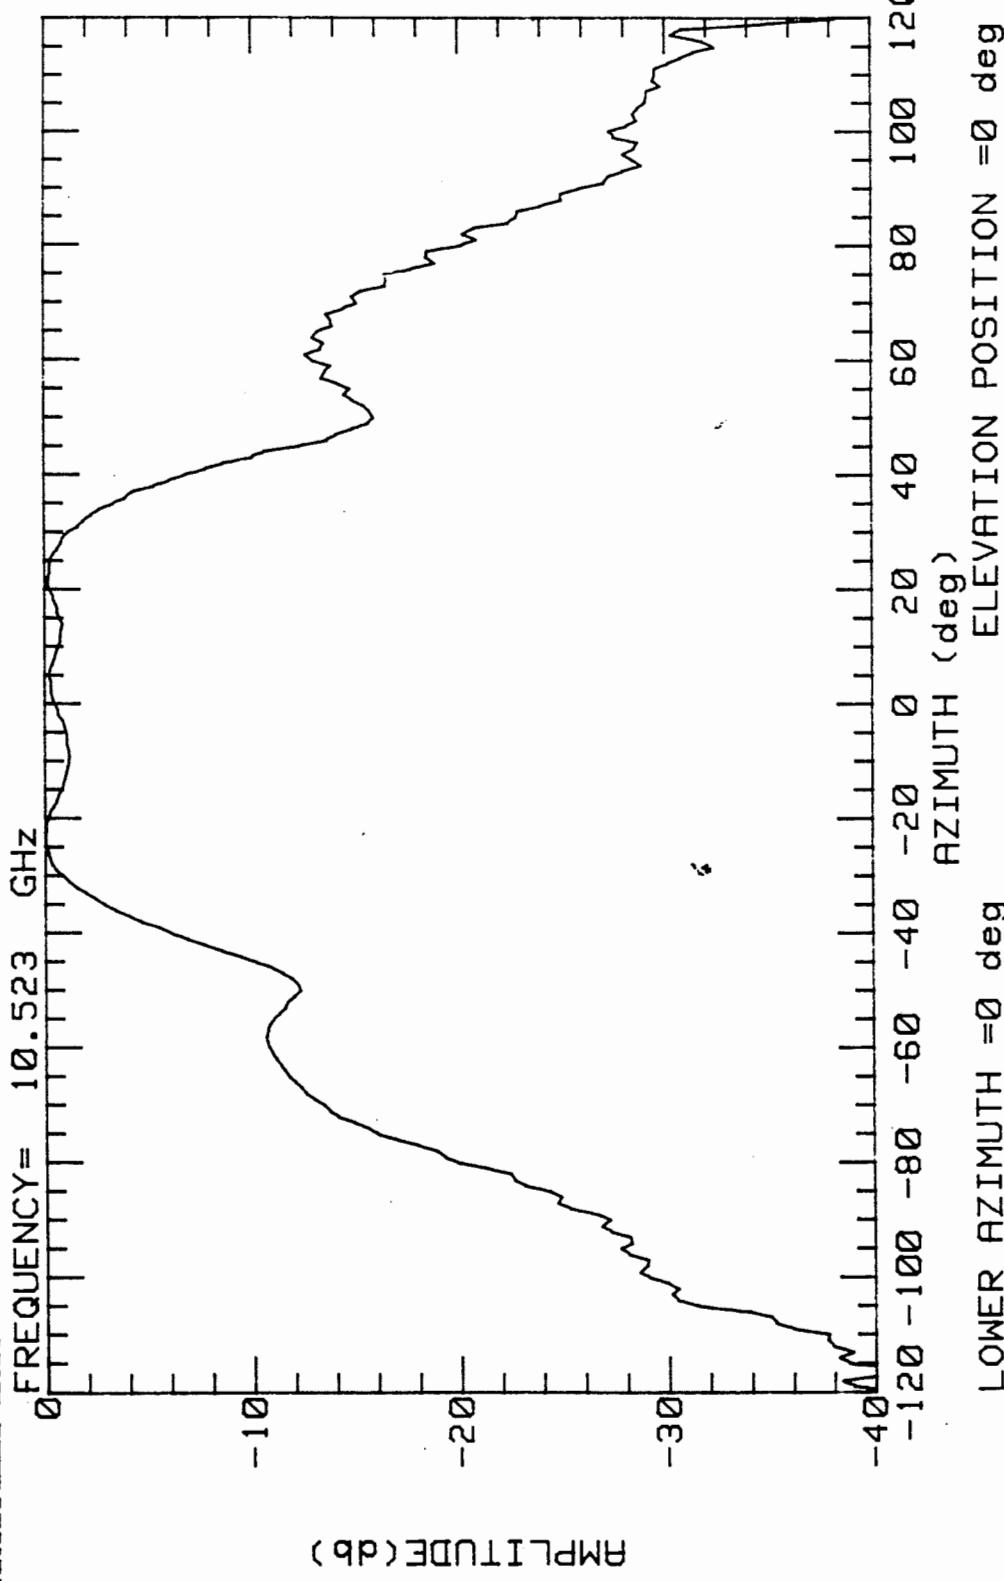


TRIBAR
Technologies Inc.

RADIATION PATTERN MEASUREMENT

TRIBAR INDUSTRIES MUNI QUIP T3 #55060 ~27
6 INCH SPACING Rx H

FREQUENCY = 10.523 GHz

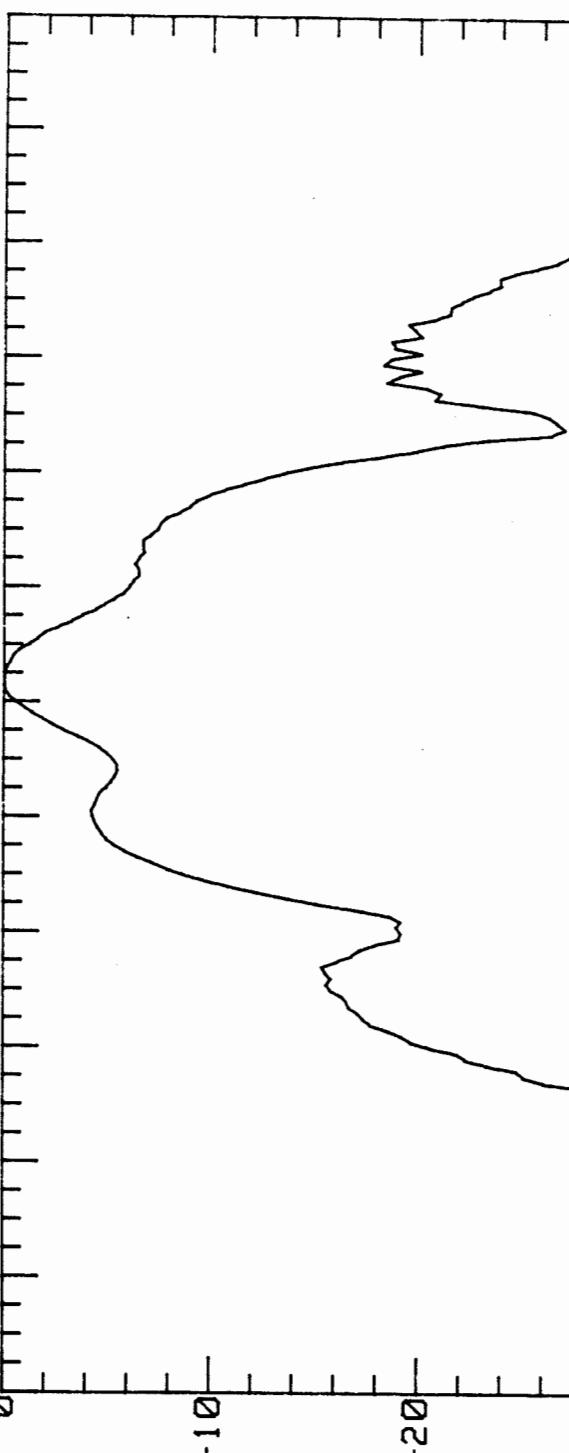


AMPLITUDE (db)

-120 -100 -80 -60 -40 -20 0 20 40 60 80 100 120
AZIMUTH (deg)
LOWER AZIMUTH = 0 deg
ELEVATION POSITION = 0 deg

MPB
Technologies Inc.

RADIATION PATTERN MEASUREMENT
TRIBAR INDUSTRIES MUNI QUIP T3 #55060 -27
2 INCH SPACING Rx V

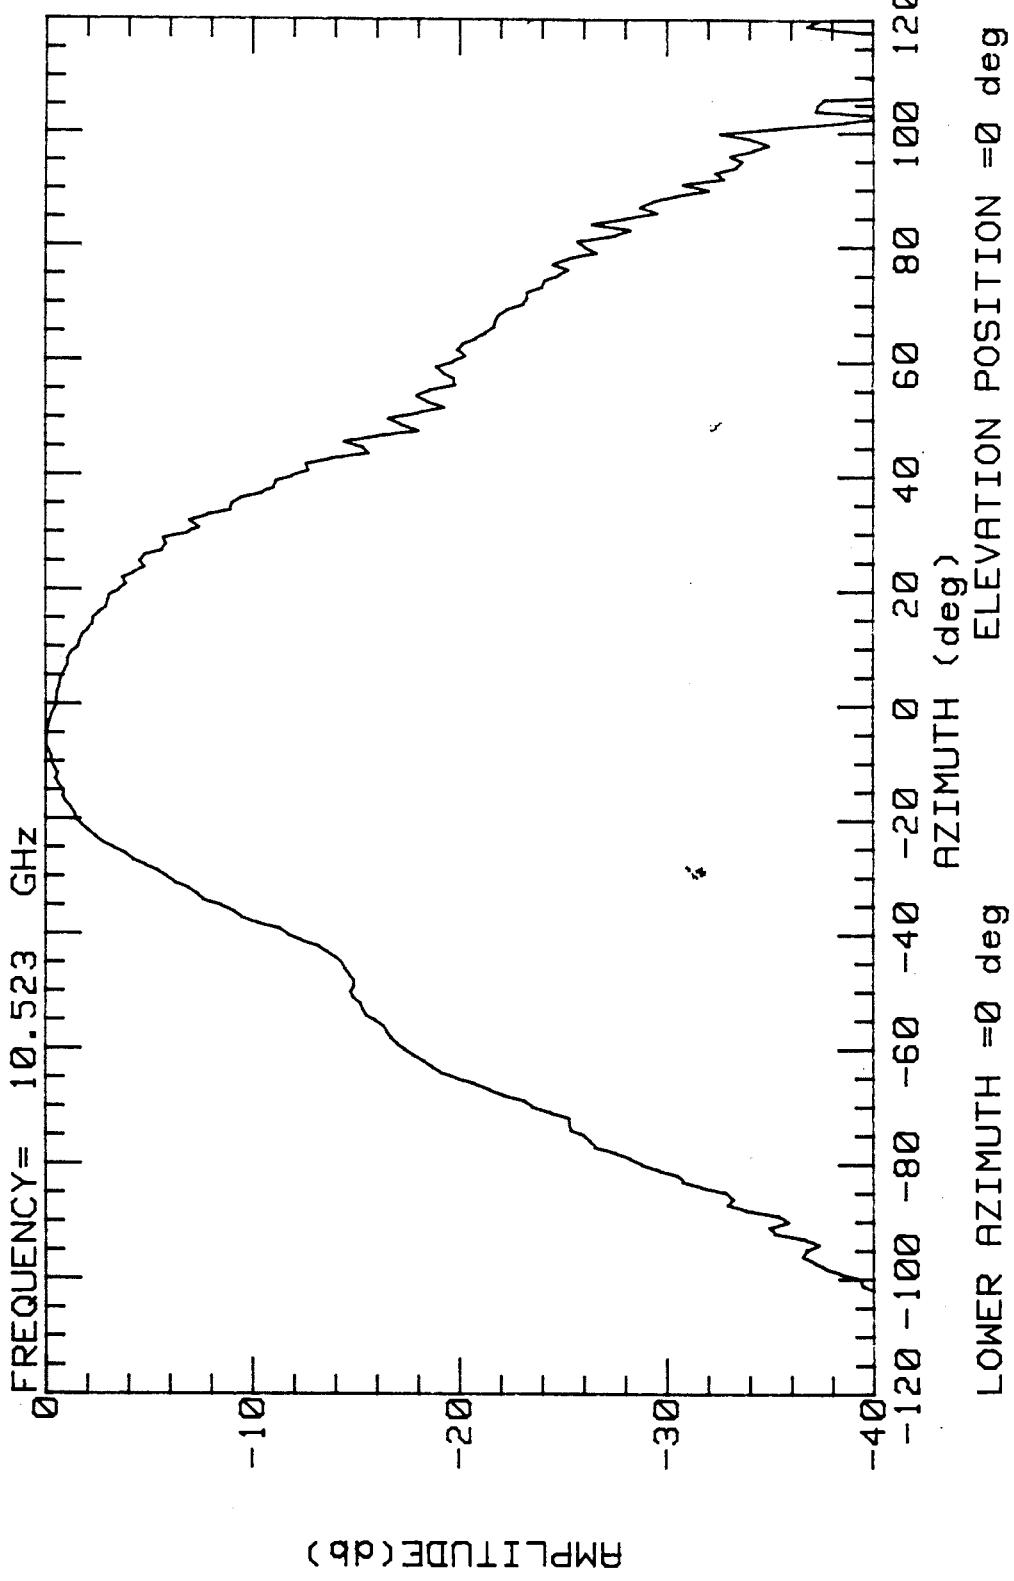


NPB
TECHNOLOGIES INC.

RADIATION PATTERN MEASUREMENT

TRIBAR INDUSTRIES MUNI QUIP T3 #55060 -2.7
6 INCH SPACING Rx V


FREQUENCY = 10.523 GHz

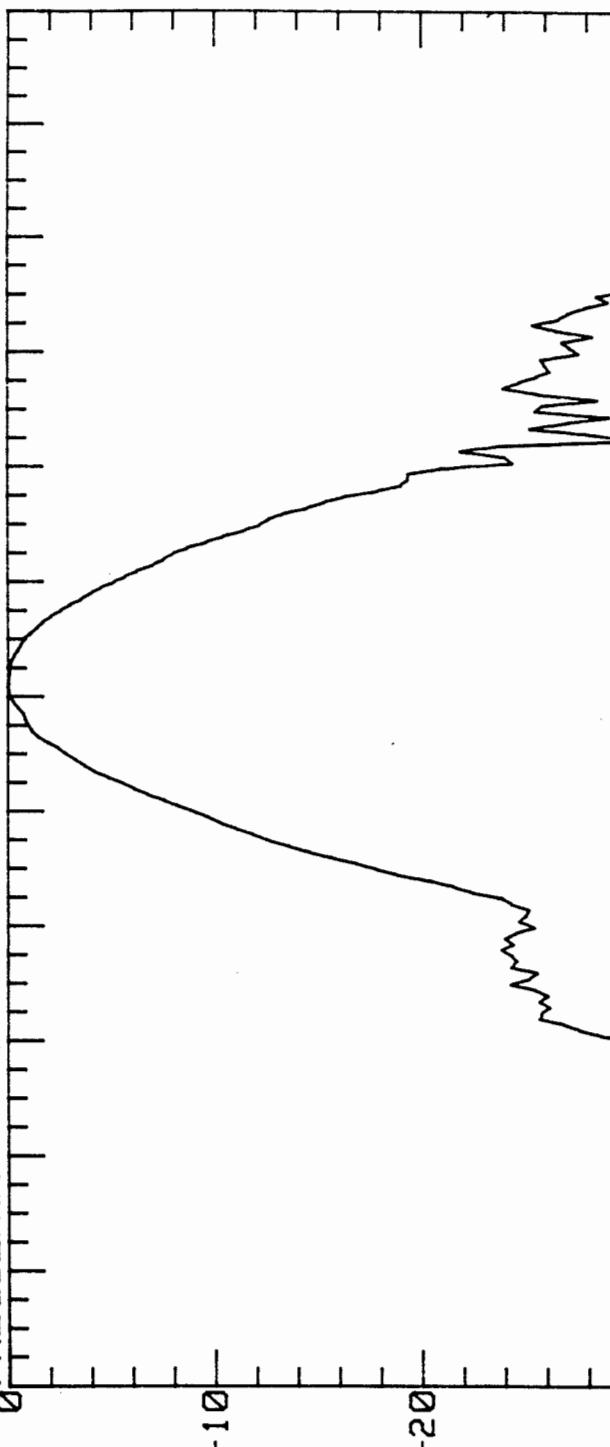

AMPLITUDE (dB)

-120 -100 -80 -60 -40 -20 0 20 40 60 80 100 120
AZIMUTH (deg)
LOWER AZIMUTH = 0 deg
ELEVATION POSITION = 0 deg

APPENDIX C



TEST EQUIPMENT REPORT

Test Comp./Part: Ottawa Police Recalls Crim

Test Technologist: L. ALLAN

Manufacturer	Description	Model	Serial #	Calib.	Recalib.
HEWLETT-PACKARD	SPECTRUM ANALYZER	1185662	2816196545 2747165464	12/16/00	12/16/02
HEWLETT-PACKARD	NETWARE ANALYZER	1851019	61554	12/16/00	12/16/02
LIAISON	ATTENUEATOR 16 DB	1950271	N/A	12/16/00	12/16/02
LIAISON	ATTENUATOR 10 DB	1950276	N/A	12/16/00	12/16/02
LEADER	PROBE	43212	2130A035		
LEADER	METER	647782	12/16/00		
LEADER	METER	647783	12/16/00		
LEADER	TEST EQUIP	1169100	12/16/00		
SCIENTIFIC INSTRUMENTS	IMAGING CARD	114-3	1042100		
SCIENTIFIC INSTRUMENTS	MAIN CARD	14-5	12/16/00		
SCIENTIFIC INSTRUMENTS	MAIN CARD	14-7	12/16/00		
SCIENTIFIC INSTRUMENTS	MAIN CARD	14-9	12/16/00		

Customer No.: 14-500

MPBT No.: 14-5

Date: Dec 23 2001

Page / of ?


TEST EQUIPMENT REPORT

Test Comp./Part:Officer Police Officer (Units)

Test Technologist: L: ALLAN

Manufacturer	Description	Model	Serial #	Calib.	Recalib.
PHD	Transit	3203	238		
HORNIGSON LTD INC	Power Corp Supply	565-10	318		
SCIENTIFIC INSTRUMENTS	IR Transistor Detector	11212-31	29		
ARCO	Convection Oven		3		
PHD	Transistor	3203	446		
TECHNICON	Auto. Densitometer	2200-10	26		
SCIENTIFIC INSTRUMENTS	Resistivity meter	100-701	18738		
HECET INSTRUMENTS	Conductometer	276	2432002482		

APPENDIX D



BIBLIOGRAPHY

- NBS:** Technical Note 1319,
"Generation of Standard Electromagnetic Fields in a
TEM Cell",
Ref: Kanda, M.; Orr, R. David
- NRCC:** "Measurement of Antenna Factors with a TEM Cell",
Ref: Kashyap, S.C.
- ECSM:** "The Equivalent Capacitance Substitution Method",
Ref: Jordan, E.C., "EM Waves & Radiating System",
p. 483
Ref: Navship 94810, "The Radio Freq. Interference
Meter", Univ. of Penn., 1962,
Para. 12.4.1
- IEEE 302-1969** "The Institute of Electrical & Electronic Engineers",
Sect. 2.2.2.3
- NBS:** Technical Note 1309, 1987
"Calibration Procedures for Horizontal Dipole Antennas
(25 to 1000 MHz)",
Ref: Camell, D.G.; Larsen, E.B.; Cruz, J.E.
- ANSI C63.5:** "American National Standards for Electromagnetic
Compatibility, Radiated Emission Measurement in EMI,
Calibration of Antennas",
1988
- SAE-ARP 958:** "Broadband Electromagnetic Interference Measurement
Antennas; Standard Calibration Requirements &
Methods
- SAFETY CODE - 6** "Recommended Safety Procedures for the Installation
and Use of Radiofrequency & Microwave Devices in
the Frequency Range 100 MHz - 300 GHz",
Environmental Health Directorate,
Health Protection Branch,
1979

